



TEST REPORT IEC 60529 Degrees of protection provided by enclosures (IP Code)	
Report Number :	221107184GZU-003
Date of issue	13 Mar 2023
Total number of pages	15
Name of Testing Laboratory preparing the Report	Intertek Testing Services Shenzhen Ltd. Guangzhou Branch
Applicant's name	Uni-Trend Technology (China) Co., Ltd
Address :	No.6, Gong Ye Bei 1st Road Songshan Lake National High-Tech Industrial Development Zone, Dongguan City Guangdong Province, China
Test specification:	
Standard	IEC 60529:1989+A1:1999+A2:2013
Test procedure :	Test report
Non-standard test method	N/A
Test Report Form No. :	IEC 60529_2013a
Test Report Form(s) Originator :	Intertek © 2019
Dated	2019-8
General disclaimer:	
<p>The test results presented in this report relate only to the object tested. Determination of the test conclusion is based on IEC Guide 115 in consideration of measurement uncertainty.</p> <p>This report is for the exclusive use of Intertek's Client and is provided pursuant to the agreement between Intertek and its Client. Intertek's responsibility and liability are limited to the terms and conditions of the agreement. Intertek assumes no liability to any party, other than to the Client in accordance with the agreement, for any loss, expense or damage occasioned by the use of this report. Only the Client is authorized to permit copying or distribution of this report and then only in its entirety. Any use of the Intertek name or one of its marks for the sale or advertisement of the tested material, product or service must first be approved in writing by Intertek. The observations and test results in this report are relevant only to the sample tested. This report by itself does not imply that the material, product, or service is or has ever been under an Intertek certification program.</p> <p>The test report only allows to be revised only within the report defined retention period unless standard or regulation was withdrawn or invalid.</p>	

Test item description :	AC Digital Power Clamp Meter	
Trade Mark :	UNI-T	
Manufacturer	Same as applicant	
Model/Type reference :	UT219P	
Ratings :	Measurement: CAT III 1000V, CAT IV 600V, 1000A~ Powered: 3 x 1.5V LR03 (or 1.2V rechargeable Ni-MH) AAA batteries IP54	
Responsible Testing Laboratory (as applicable), testing procedure and testing location(s):		
<input checked="" type="checkbox"/>	Testing Laboratory:	Intertek Testing Services Shenzhen Ltd. Guangzhou Branch
Testing location/ address	Intertek Testing Services Shenzhen Ltd. Guangzhou Branch Room 02, & 101/E201/E301/E401/E501/E601/E701/E801 of Room 01 1-8/F., No. 7-2. Caipin Road, Science City, GETDD, Guangzhou, Guangdong, China	
Tested by (name, function, signature) :	Eric Deng / Engineer	
Approved by (name, function, signature) .. :	Justin He / Manager	


List of Attachments (including a total number of pages in each attachment): Appendix 1: Product photos 2 pages	
Summary of testing: This product under test complied with IEC 60529:1989+A1:1999+A2:2013.	
Tests performed (name of test and test clause): All applicable clauses were performed.	Testing location: Intertek Testing Services Shenzhen Ltd. Guangzhou Branch Room 02, & 101/E201/E301/E401/E501/E601/E701/E801 of Room 01 1-8/F., No. 7-2. Caipin Road, Science City, GETDD, Guangzhou, Guangdong, China

Copy of marking plate:

1. Marking on main part



2. Marking on battery cover

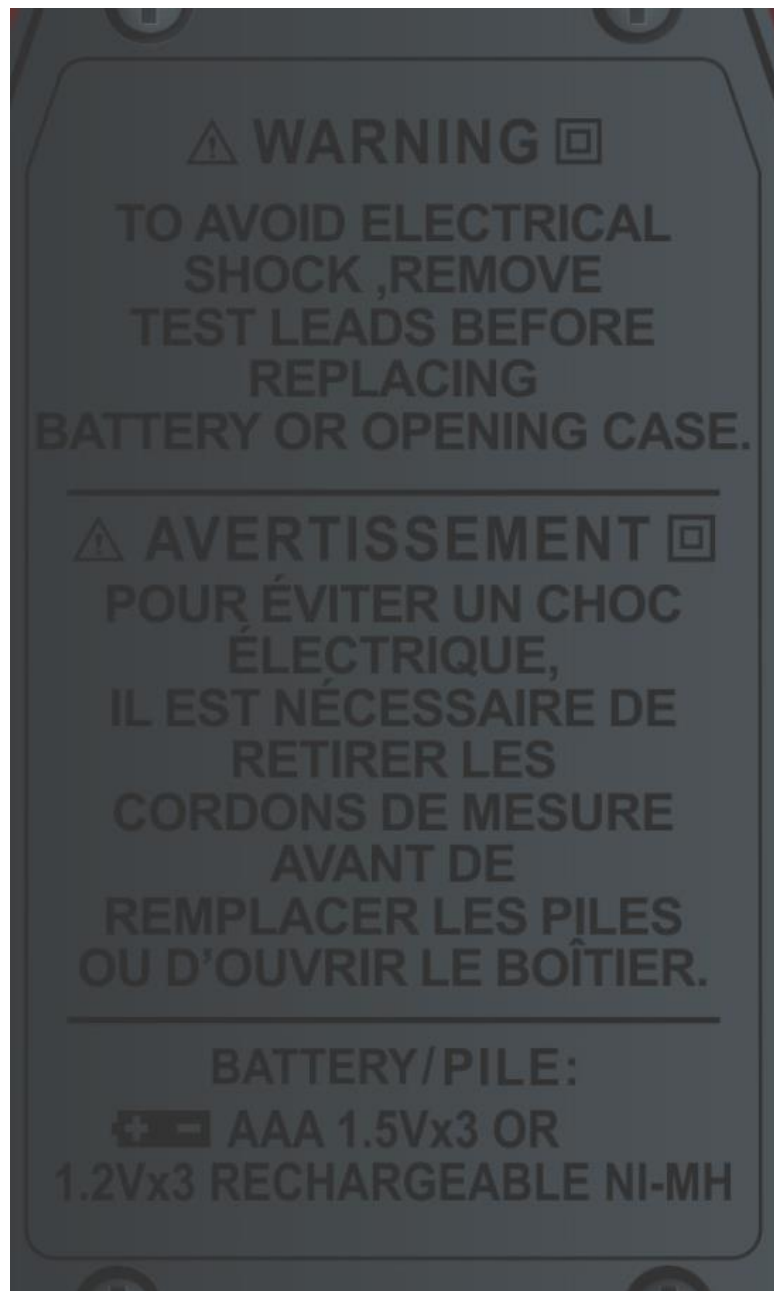

<p>Possible test case verdicts:</p> <ul style="list-style-type: none">- test case does not apply to the test object.....: N/A- test object does meet the requirement.....: P (Pass)- compliance with the requirement not evaluated..: N/E (Not Evaluated)- test object does not meet the requirement.....: F (Fail)
<p>Testing.....:</p> <p>Date of receipt of test item: 7 Nov 2022</p> <p>Date (s) of performance of tests: 7 Nov 2022 – 13 Mar 2023</p>
<p>General remarks:</p> <p>Throughout this report a point is used as the decimal separator.</p>
<p>Name and address of factory (ies).....: Same as applicant</p>
<p>General product information:</p> <p>UT219P is a digital power clamp with fundamental frequency up to 1 kHz. This clamp meter can be used to measure AC voltage, AC current, active power, apparent power, reactive power, power factor, phase angle, power quality, frequency, phase sequence, total harmonic distortion, harmonic component, etc. It has different measurement modes including single phase, three-phase three-wire, and three-phase four-wire. Designed with Bluetooth function, measurement data can be monitored and recorded via mobile phone and tablet, and professional report can be generated. Featuring easy operation, stable performance, accurate measurement and more, UT219P can be applied in multiple fields such as:</p> <ol style="list-style-type: none">1) Measure power quality of UPS to evaluate if operation is normal.2) Measure power factor of power system to analyze capacitive or inductive load.3) Measure harmonic of power grid of power system, to find out harmonic issue that may damage the load of nonlinear equipment of power grid.4) Troubleshoot 400Hz AC power supply system of aviation and 25Hz AC power supply system of railway.5) Test and maintain high-power motor, centrifugal fan, centrifugal water pump, wind power generation, solar power generation.6) Test new energy vehicles and hybrid electric vehicles, evaluate motor efficiency, inverter efficiency and energy consumption of driving.

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict
11	General requirements for tests		P
11.1	Atmospheric conditions for water or dust tests		P
	Temperature range: 15 °C to 35 °C	25.5°C	--
	Relative humidity: 25 % to 75 %	66.2%	--
	Air pressure: 86 kPa to 106 kPa	101kPa	--
11.2	Test samples		P
	the number of samples to be tested	Two	P
	conditions for mounting,		P
	the pre-conditioning, if necessary	Not pre-conditioning	N/A
	whether to be tested energized or not;	Not energized	N/A
	whether to be tested with its parts in motion or not.		N/A
11.3	Application of test requirements and interpretation of test results	This standard applied	P
11.4	Combination of test conditions for the first characteristic numeral		P
	access to hazardous parts	No hazardous part	N/A
	solid foreign objects	Dust-tight	P
11.5	Empty enclosures	Integrity unit	N/A
12	Tests for protection against access to hazardous parts indicated by the first characteristic numeral		N/A
12.1, 12.2	Access probes, Test conditions	No hazardous part	N/A
	First numeral 1, or additional letter A Sphere 50 mm diameter, test force 50 N ± 10 %		N/A
	First numeral 2, or additional letter B Jointed test finger, test force 10 N ± 10 %		N/A
	First numeral 3, or additional letter C Test rod 2,5 mm diameter, 100 mm long, test force 3 N ± 10 %		N/A
	First numeral 4,5,6, or additional letter D Test wire 1,0 mm diameter, 100 mm long, test force 1 N ± 10 %		P
12.3	Acceptance conditions		P
12.3.1	For low-voltage equipment (rated voltages not exceeding 1 000 V a.c. and 1 500 V d.c.), the access probe shall not touch hazardous live parts.		P

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict
12.3.2	For high-voltage equipment (rated voltages exceeding 1 000 V a.c. and 1 500 V d.c.), when the access probe is placed in the most unfavourable position(s), the equipment shall be capable of withstanding the dielectric tests as specified in the relevant product standard applicable to the equipment.		N/A
12.3.3	For equipment with hazardous mechanical parts, the access probe shall not touch hazardous mechanical parts.	No such part	N/A
13	Tests for protection against solid foreign objects indicated by the first characteristic numeral		P
13.1	Test means		P
13.2	Test conditions for first characteristic numerals 1, 2, 3, 4	IP5X	N/A
	First characteristic numeral 1, with rigid sphere without handle or guard 50 0 mm diameter, force 50 N ± 10 %		N/A
	First characteristic numeral 2, with rigid sphere without handle or guard 12,5 mm diameter, force 30 N ± 10 %		N/A
	First characteristic numeral 3, with rigid steel rod 2,5 mm diameter with edges free from burrs, force 3 N ± 10 %		N/A
	First characteristic numeral 4, with rigid steel rod 1,0 mm diameter with edges free from burrs, force 1 N ± 10 %		N/A
13.3	Acceptance conditions for first characteristic numerals 1, 2, 3, 4, the protection is satisfactory if the full diameter of the probe specified does not pass through any opening.		N/A
13.4	Dust test for first characteristic numerals 5 and 6		P
	The test is made using a dust chamber incorporating the basic principles shown in figure 2 whereby the powder circulation pump may be replaced by other means suitable to maintain the talcum powder in suspension in a closed test chamber. The talcum powder used shall be able to pass through a square-meshed sieve the nominal wire diameter of which is 50 µm and the nominal width of a gap between wires 75 µm. The amount of talcum powder to be used is 2 kg per cubic meter of the test chamber volume. It shall not have been used for more than 20 tests.		P

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict
Category 1:	<p>Enclosures where the normal working cycle of the equipment causes reductions in air pressure within the enclosure below that of the surrounding air, for example, due to thermal cycling effects.</p> <p>The enclosure under test is supported inside the test chamber and the pressure inside the enclosure is maintained below the surrounding atmospheric pressure by a vacuum pump.</p> <p>The object of the test is to draw into the enclosure, by means of depression, a volume of air 80 times the volume of the sample enclosure tested without exceeding the extraction rate of 60 volumes per hour. In no event shall the depression exceed 2 kPa (20 mbar) on the manometer</p>	Category 2 used	N/A
	If an extraction rate of 40 to 60 volumes per hour is obtained the duration of the test is 2 h.		N/A
	If, with a maximum depression of 2 kPa (20 mbar), the extraction rate is less than 40 volumes per hour, the test is continued until 80 volumes have been drawn through, or a period of 8 h has elapsed.		N/A
Category 2:	<p>Enclosures where no pressure difference relative to the surrounding air is present.</p> <p>The enclosure under test is supported in its normal operating position inside the test chamber but is not connected to a vacuum pump. Any drain-hole normally open shall be left open for the duration of the test. The test shall be continued for a period of 8 h.</p>		P
13.5	Special conditions for first characteristic numeral 5		P
13.5.1	The enclosure shall be deemed category 1 unless the relevant product standard for the equipment specifies that the enclosure is category 2.		P
13.5.2	The protection is satisfactory if, on inspection, talcum powder has not accumulated in a quantity or location such that, as with any other kind of dust, it could interfere with the correct operation of the equipment or impair safety.		P
13.6	Special conditions for first characteristic numeral 6		N/A

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict
13.6.1	The enclosure shall be deemed category 1, whether reductions in pressure below the atmospheric pressure are present or not.		N/A
13.6.2	The protection is satisfactory if no deposit of dust is observable inside the enclosure at the end of the test.		N/A
14	Tests for protection against water indicated by the second characteristic numeral		P
14.1	Test means		P
14.2	Test condition		P
	The tests are conducted with fresh water.		P
	During the tests for IPX1 to IPX6 the water temperature should not differ by more than 5 K from the temperature of the specimen under test.	Water :24.4°C Equipment: 25.1°C	P
	For IPX7 and IPX9 details of the water temperature are given in 14.2.7 and 14.2.9 respectively.		N/A
	During the test, the moisture contained inside the enclosure may partly condense. The dew which may thus deposit shall not be mistaken for an ingress of water		P
	For the purpose of the tests, the surface area of the enclosure is calculated with a tolerance of 10 %.		P
	Adequate safety precautions should be taken when testing the equipment in the energized condition.	Not energized	N/A
14.2.1	Test for second characteristic numeral 1 with the drip box	IPX4	N/A
	The turntable on which the enclosure is placed has a rotation speed of 1 r/min and the eccentricity (distance between turntable axis and specimen axis) is approximately 100 mm.		N/A
	An enclosure normally fixed to a wall or ceiling is fixed in its normal position of use to a wooden board		N/A
	The enclosure under test is placed in its normal operating position under the drip box,		N/A
	Water flow rate 1 mm/min. The duration of test is 10 min.		N/A
14.2.2	Test for second characteristic numeral 2 with the drip box	IPX4	N/A

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict
	The table on which the enclosure is placed does not turn. These positions are 15° on either side of the vertical in two mutually perpendicular planes		N/A
	Water flow rate 1 mm/min. The enclosure is tested for 2,5 min in each of four fixed positions of tilt. The total duration of the test is 10 min.		N/A
14.2.3	Test for second characteristic numeral 3 with oscillating tube or spray nozzle	IPX4	N/A
a) oscillating tube	Water flow rate 0,07 l/min ± 5 % per hole, multiplied by number of holes		N/A
	Spray ± 60° from vertical, distance max. 200 mm		N/A
	The enclosure to be tested is placed at the centre point of the semicircle. The tube is caused to oscillate through an angle of 120°, 60° on either side of the vertical, the time for one complete oscillation (2 × 120°) being about 4 s and the test duration being 5 min.		N/A
	The enclosure is then turned through a horizontal angle of 90° and the test is continued for a further 5 min.		N/A
b) spray nozzle	Water flow rate 10 l/min ± 5 %		N/A
	Spray ± 60° from vertical		N/A
	The test duration is 1 min/m ² of the calculated surface area of the enclosure (excluding any mounting surface), with a minimum duration of 5 min.		N/A
14.2.4	Test for second characteristic numeral 4 with oscillating tube or spray nozzle	IPX4	P
a) oscillating tube	Water flow rate 0,07 l/min ± 5 % per hole, multiplied by number of holes		P
	The oscillating tube has spray holes over the whole 180° of the semicircle.		P
	The tube is caused to oscillate through an angle of almost 360°, 180° on either side of the vertical, the time for one complete oscillation (2 × 360°) being about 12 s.		P
	The duration of the test is 10 min.		P
b) spray nozzle	Water flow rate 10 l/min ± 5 %		N/A
	Spray ± 180° from vertical		N/A

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict
	The test duration is 1 min/m ² of the calculated surface area of the enclosure (excluding any mounting surface), with a minimum duration of 5 min.		N/A
14.2.5	Test for second characteristic numeral 5 with the 6,3 mm nozzle	IPX4	N/A
	delivery rate: 12,5 l/min ± 5 %;		N/A
	core of the substantial stream: circle of approximately 40 mm diameter at 2,5 m distance from nozzle;		N/A
	test duration per square metre of enclosure surface area likely to be sprayed: 1 min; minimum test duration: 3 min;		N/A
	distance from nozzle to enclosure surface: between 2,5 m and 3 m.		N/A
14.2.6	Test for second characteristic numeral 6 with the 12,5 mm nozzle	IPX4	N/A
	delivery rate: 100 l/min ± 5 %;		N/A
	core of the substantial stream: circle of approximately 120 mm diameter at 2,5 m distance from nozzle;		N/A
	test duration per square metre of enclosure surface area likely to be sprayed: 1 min; minimum test duration: 3 min;		N/A
	distance from nozzle to enclosure surface: between 2,5 m and 3 m.		N/A
14.2.7	Test for second characteristic numeral 7: temporary immersion between 0,15 m and 1 m	IPX4	N/A
	the lowest point of enclosures with a height less than 850 mm is located 1 000 mm below the surface of the water		N/A
	the highest point of enclosures with a height equal to or greater than 850 mm is located 150 mm below the surface of the water;		N/A
	the duration of the test is 30 min;		N/A
	the water temperature does not differ from that of the equipment by more than 5 K.		N/A
14.2.8	Test for second characteristic numeral 8: continuous immersion subject to agreement	IPX4	N/A
	the test conditions are subject to agreement between manufacturer and user, but they shall be more severe than those prescribed in 14.2.7		N/A

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict
14.2.9	Test for second characteristic numeral 9 by high pressure and temperature water jetting	IPX4	N/A
	<p>a) For small enclosures (largest dimension less than 250 mm), the enclosure shall be mounted on the test device shown in Figure 12.</p> <ul style="list-style-type: none"> - turntable speed: 5 r/min \pm 1 r/min - spray positions: 0°, 30°, 60°, 90° <p>The test duration is 30 s per position.</p>		N/A
	<p>b) For large enclosures (largest dimension greater than or equal to 250 mm), the enclosure shall be mounted as per intended use. The entire exposed surface area of the enclosure shall be subjected to the spray at some point during the test procedure.</p> <ul style="list-style-type: none"> - spray positions: the enclosure shall be sprayed from all practical directions covering the entire surface area and the spray shall be, as far as possible, perpendicular to the sprayed surface. - distance between nozzle and sample under test shall be 175 \pm 25 mm. <p>The test duration is 1 min/m² of the calculated surface area of the enclosure (excluding any mounting surface), with a minimum duration of 3 min.</p>		N/A
14.3	Acceptance conditions		P
	<p>In general, if any water has entered, it shall not:</p> <ul style="list-style-type: none"> - be sufficient to interfere with the correct operation of the equipment or impair safety; - deposit on insulation parts where it could lead to tracking along the creepage distances; - reach live parts or windings not designed to operate when wet; - accumulate near the cable end or enter the cable if any. 	No water has entered	P
	<p>If the enclosure is provided with drain-holes, it should be proved by inspection that any water which enters does not accumulate and that it drains away without doing any harm to the equipment.</p>	No such part	N/A

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict

Appendix 1 product photo:



Photo 1 – During IP5X testing

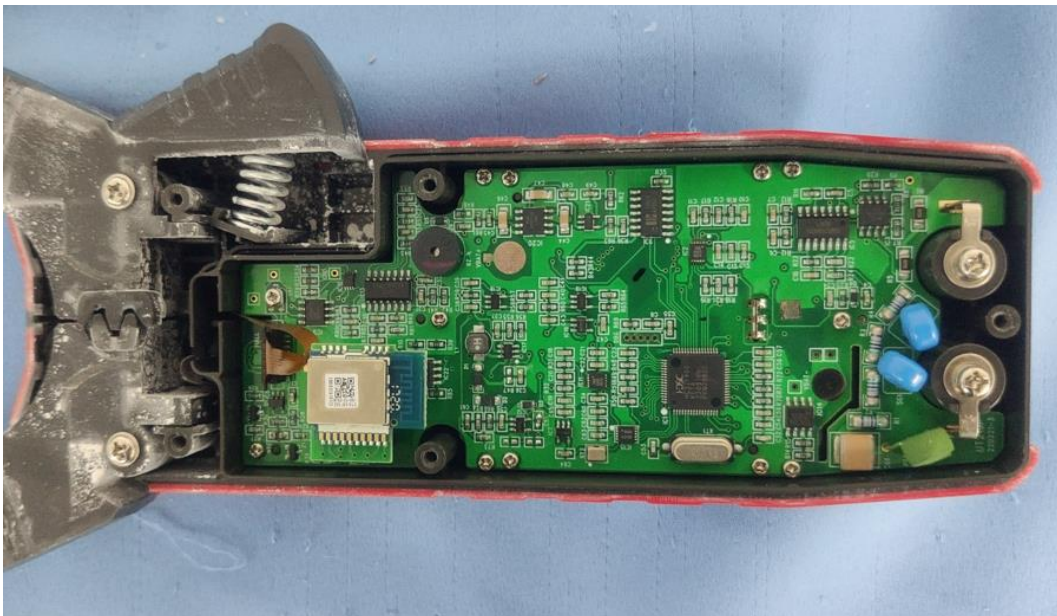


Photo 2 – After IP5X test

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict



Photo 3 – During IPX4 testing

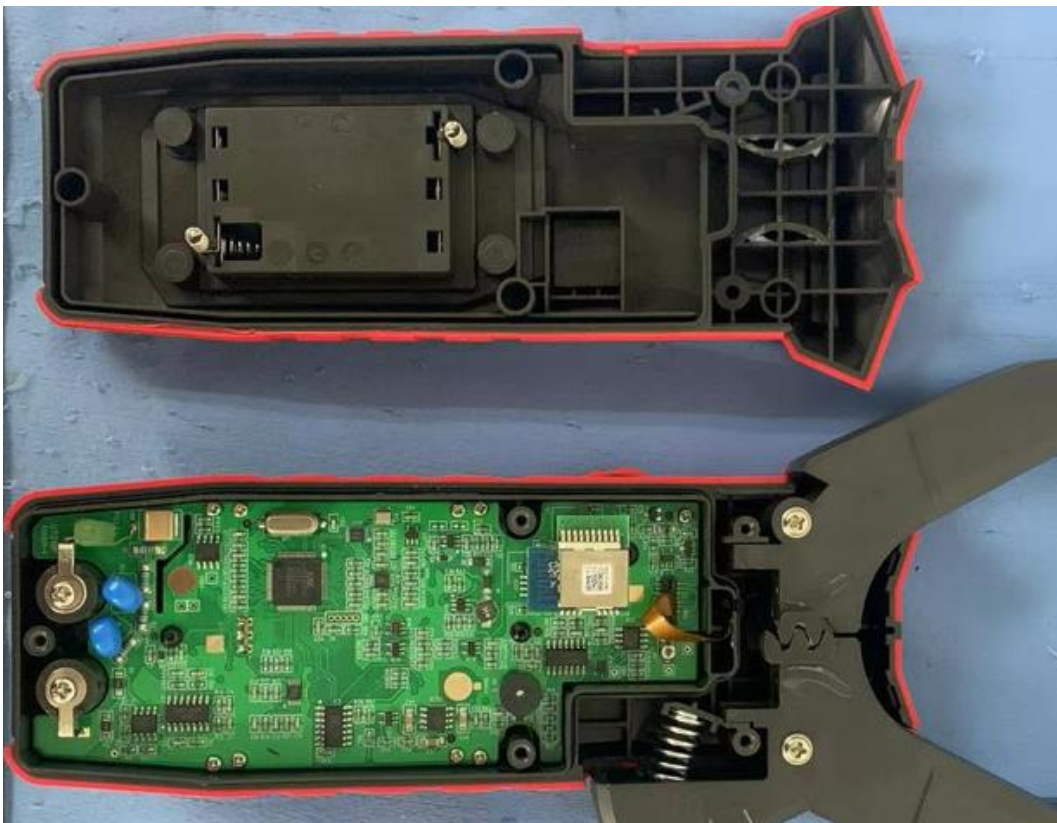


Photo 4 – After IPX4 test

****END OF REPORT****