

TEST REPORT IEC 60529 Degrees of protection provided by enclosures (IP Code)	
Report Number	231011122GZU-003
Date of issue	04 Dec 2023
Total number of pages	15
Name of Testing Laboratory preparing the Report	Intertek Testing Services Shenzhen Ltd. Guangzhou Branch
Applicant's name	Uni-Trend Technology (China) Co., Ltd
Address	No. 6, Gong Ye Bei 1st Road, Songshan Lake National High-Tech Industrial Development Zone, DONGGUAN CITY Guangdong Province 523808, China
Test specification:	
Standard	IEC 60529:1989+A1:1999+A2:2013
Test procedure	Test report
Non-standard test method	N/A
Test Report Form No.	IEC 60529_2013a
Test Report Form(s) Originator	Intertek © 2019
Dated	2019-8
General disclaimer:	
<p>The test results presented in this report relate only to the object tested. Determination of the test conclusion is based on IEC Guide 115 in consideration of measurement uncertainty.</p> <p>This report is for the exclusive use of Intertek's Client and is provided pursuant to the agreement between Intertek and its Client. Intertek's responsibility and liability are limited to the terms and conditions of the agreement. Intertek assumes no liability to any party, other than to the Client in accordance with the agreement, for any loss, expense or damage occasioned by the use of this report. Only the Client is authorized to permit copying or distribution of this report and then only in its entirety. Any use of the Intertek name or one of its marks for the sale or advertisement of the tested material, product or service must first be approved in writing by Intertek. The observations and test results in this report are relevant only to the sample tested. This report by itself does not imply that the material, product, or service is or has ever been under an Intertek certification program.</p> <p>The test report only allows to be revised only within the report defined retention period unless standard or regulation was withdrawn or invalid.</p>	

Test item description :	Professional AC/DC Clamp Meter-SOLAR
Trade Mark :	UNI-T
Manufacturer	Same as applicant
Model/Type reference :	UT219PV
Ratings :	Powered: 2 x 1.5V AA batteries Measurement: CAT III 1500V, CAT IV 600V, 1000A Rated voltage of measurement terminals: 2500 Vdc, 1500 Vac IP65

Responsible Testing Laboratory (as applicable), testing procedure and testing location(s):		
<input checked="" type="checkbox"/>	Testing Laboratory:	Intertek Testing Services Shenzhen Ltd. Guangzhou Branch
	Testing location/ address	Room 101/301/401/102/202/302/402/502/602/702/802, No. 7-2, Caipin Road, Huangpu District, Guangzhou, Guangdong, China
	Tested by (name, function, signature) :	Bin Zhong, Engineer 
	Approved by (name, function, signature) ..:	Justin He, Manager 

List of Attachments (including a total number of pages in each attachment):

Appendix 1: Product photos

2 pages

Summary of testing:

This product under test complied with IEC 60529: 1989 + A1: 1999 + A2: 2013 + Corr.1 2013 + Corr2: 2015 + AMD2:2013/Corr1: 2019 and EN 60529:1991+A1:2000+A2:2013+AC:2016+A2:2013/AC 2019.

Tests performed (name of test and test clause):

All applicable clauses were performed.

Testing location:

Intertek Testing Services Shenzhen Ltd. Guangzhou Branch
Room
101/301/401/102/202/302/402/502/602/702/802,
No. 7-2, Caipin Road, Huangpu District,
Guangzhou, Guangdong, China

Copy of marking plate:

The artwork below may be only a draft. The use of certification marks on a product must be authorized by the respective NCBs that own these marks.



Possible test case verdicts:	
- test case does not apply to the test object	: N/A
- test object does meet the requirement	: P (Pass)
- compliance with the requirement not evaluated..:	: N/E (Not Evaluated)
- test object does not meet the requirement	: F (Fail)
Testing	
Date of receipt of test item	: 11 Oct 2023
Date (s) of performance of tests.....	: 11 Oct 2023 – 20 Nov 2023
General remarks:	
<p>Throughout this report a point is used as the decimal separator.</p> <p>Determination of the test conclusion is based on IEC Guide 115 in consideration of measurement uncertainty. This report is for the exclusive use of Intertek's Client and is provided pursuant to the agreement between Intertek and its Client. Intertek's responsibility and liability are limited to the terms and conditions of the agreement. Intertek assumes no liability to any party, other than to the Client in accordance with the agreement, for any loss, expense or damage occasioned by the use of this report. Only the Client is authorized to permit copying or distribution of this report and then only in its entirety. Any use of the Intertek name or one of its marks for the sale or advertisement of the tested material, product or service must first be approved in writing by Intertek. The observations and test results in this report are relevant only to the sample tested. This report by itself does not imply that the material, product, or service is or has ever been under an Intertek certification program.</p> <p>The test report only allows to be revised only within the report defined retention period unless standard or regulation was withdrawn or invalid.</p>	
Name and address of factory (ies).....	: Same as applicant
General product information:	
<p>UT219PV is a True-RMS AC/DC clamp meter specially designed for photovoltaic high-voltage environments. It can be used to measure AC/DC voltage (2500VDC, 1500Vac for floating voltage in no measurement category circuit), AC/DC current, LPF voltage/current, inrush current, peak current, DC power, flex current sensor, resistance, continuity, diode, capacitance, temperature, and more. UT219PV has data storage function and Bluetooth function, which enable remote control and monitoring on the measurement data via the "UNI-T Smart Measure" APP. UT219PV is an ideal meter for the installation and maintenance in photovoltaic field. This Clamp Meter can also be applied in the energy storage system, UPS (uninterrupted power supply), large-scale motor, and other high voltage environments.</p>	

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict
11	General requirements for tests		P
11.1	Atmospheric conditions for water or dust tests		P
	Temperature range: 15 °C to 35 °C	23.2°C	--
	Relative humidity: 25 % to 75 %	58.9%	--
	Air pressure: 86 kPa to 106 kPa	101kPa	--
11.2	Test samples		P
	the number of samples to be tested	Two	P
	conditions for mounting,		P
	the pre-conditioning, if necessary	Not pre-conditioning	P
	whether to be tested energized or not;	Not energized	N/A
	whether to be tested with its parts in motion or not.		N/A
11.3	Application of test requirements and interpretation of test results	This standard applied	P
11.4	Combination of test conditions for the first characteristic numeral		P
	access to hazardous parts	The test wire of 1,0 mm was not penetrate and adequate clearance was be kept	P
	solid foreign objects	Dust-tight	P
11.5	Empty enclosures	Integrity unit	N/A
12	Tests for protection against access to hazardous parts indicated by the first characteristic numeral		P
12.1, 12.2	Access probes, Test conditions		P
	First numeral 1, or additional letter A Sphere 50 mm diameter, test force 50 N ± 10 %		N/A
	First numeral 2, or additional letter B Jointed test finger, test force 10 N ± 10 %		N/A
	First numeral 3, or additional letter C Test rod 2,5 mm diameter, 100 mm long, test force 3 N ± 10 %		N/A
	First numeral 4,5,6, or additional letter D Test wire 1,0 mm diameter, 100 mm long, test force 1 N ± 10 %		P
12.3	Acceptance conditions		P

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict
12.3.1	For low-voltage equipment (rated voltages not exceeding 1 000 V a.c. and 1 500 V d.c.), the access probe shall not touch hazardous live parts.	CAT III 1500V, CAT IV 600V, 1	P
12.3.2	For high-voltage equipment (rated voltages exceeding 1 000 V a.c. and 1 500 V d.c.), when the access probe is placed in the most unfavourable position(s), the equipment shall be capable of withstanding the dielectric tests as specified in the relevant product standard applicable to the equipment.	Rated voltage of measurement terminals: 2500 Vdc, 1500 Vac	P
12.3.3	For equipment with hazardous mechanical parts, the access probe shall not touch hazardous mechanical parts.	No such part	N/A
13	Tests for protection against solid foreign objects indicated by the first characteristic numeral		P
13.1	Test means	IP6X	P
13.2	Test conditions for first characteristic numerals 1, 2, 3, 4		N/A
	First characteristic numeral 1, with rigid sphere without handle or guard 50 0 mm diameter, force 50 N ± 10 %		N/A
	First characteristic numeral 2, with rigid sphere without handle or guard 12,5 mm diameter, force 30 N ± 10 %		N/A
	First characteristic numeral 3, with rigid steel rod 2,5 mm diameter with edges free from burrs, force 3 N ± 10 %		N/A
	First characteristic numeral 4, with rigid steel rod 1,0 mm diameter with edges free from burrs, force 1 N ± 10 %		N/A
13.3	Acceptance conditions for first characteristic numerals 1, 2, 3, 4, the protection is satisfactory if the full diameter of the probe specified does not pass through any opening.		N/A
13.4	Dust test for first characteristic numerals 5 and 6	IP6X	P

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict
	The test is made using a dust chamber incorporating the basic principles shown in figure 2 whereby the powder circulation pump may be replaced by other means suitable to maintain the talcum powder in suspension in a closed test chamber. The talcum powder used shall be able to pass through a square-meshed sieve the nominal wire diameter of which is 50 um and the nominal width of a gap between wires 75 um. The amount of talcum powder to be used is 2 kg per cubic meter of the test chamber volume. It shall not have been used for more than 20 tests.		P
Category 1:	Enclosures where the normal working cycle of the equipment causes reductions in air pressure within the enclosure below that of the surrounding air, for example, due to thermal cycling effects. The enclosure under test is supported inside the test chamber and the pressure inside the enclosure is maintained below the surrounding atmospheric pressure by a vacuum pump. The object of the test is to draw into the enclosure, by means of depression, a volume of air 80 times the volume of the sample enclosure tested without exceeding the extraction rate of 60 volumes per hour. In no event shall the depression exceed 2 kPa (20 mbar) on the manometer		P
	If an extraction rate of 40 to 60 volumes per hour is obtained the duration of the test is 2 h.		P
	If, with a maximum depression of 2 kPa (20 mbar), the extraction rate is less than 40 volumes per hour, the test is continued until 80 volumes have been drawn through, or a period of 8 h has elapsed.		P
Category 2:	Enclosures where no pressure difference relative to the surrounding air is present. The enclosure under test is supported in its normal operating position inside the test chamber but is not connected to a vacuum pump. Any drain-hole normally open shall be left open for the duration of the test. The test shall be continued for a period of 8 h.	Category 1 used	P
13.5	Special conditions for first characteristic numeral 5	IP6X	N/A

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict
13.5.1	The enclosure shall be deemed category 1 unless the relevant product standard for the equipment specifies that the enclosure is category 2.		N/A
13.5.2	The protection is satisfactory if, on inspection, talcum powder has not accumulated in a quantity or location such that, as with any other kind of dust, it could interfere with the correct operation of the equipment or impair safety.		N/A
13.6	Special conditions for first characteristic numeral 6		P
13.6.1	The enclosure shall be deemed category 1, whether reductions in pressure below the atmospheric pressure are present or not.		P
13.6.2	The protection is satisfactory if no deposit of dust is observable inside the enclosure at the end of the test.		P
14	Tests for protection against water indicated by the second characteristic numeral		P
14.1	Test means		P
14.2	Test condition		P
	The tests are conducted with fresh water.		P
	During the tests for IPX1 to IPX6 the water temperature should not differ by more than 5 K from the temperature of the specimen under test.	Water :22.4°C Equipment: 23.5°C	P
	For IPX7 and IPX9 details of the water temperature are given in 14.2.7 and 14.2.9 respectively.		N/A
	During the test, the moisture contained inside the enclosure may partly condense. The dew which may thus deposit shall not be mistaken for an ingress of water		P
	For the purpose of the tests, the surface area of the enclosure is calculated with a tolerance of 10 %.		P
	Adequate safety precautions should be taken when testing the equipment in the energized condition.	Not energized	N/A
14.2.1	Test for second characteristic numeral 1 with the drip box	IPX5	N/A
	The turntable on which the enclosure is placed has a rotation speed of 1 r/min and the eccentricity (distance between turntable axis and specimen axis) is approximately 100 mm.		N/A

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict
	An enclosure normally fixed to a wall or ceiling is fixed in its normal position of use to a wooden board		N/A
	The enclosure under test is placed in its normal operating position under the drip box,		N/A
	Water flow rate 1 mm/min. The duration of test is 10 min.		N/A
14.2.2	Test for second characteristic numeral 2 with the drip box	IPX5	N/A
	The table on which the enclosure is placed does not turn. These positions are 15° on either side of the vertical in two mutually perpendicular planes		N/A
	Water flow rate 1 mm/min. The enclosure is tested for 2,5 min in each of four fixed positions of tilt. The total duration of the test is 10 min.		N/A
14.2.3	Test for second characteristic numeral 3 with oscillating tube or spray nozzle	IPX5	N/A
a) oscillating tube	Water flow rate 0,07 l/min ± 5 % per hole, multiplied by number of holes		N/A
	Spray ± 60° from vertical, distance max. 200 mm		N/A
	The enclosure to be tested is placed at the centre point of the semicircle. The tube is caused to oscillate through an angle of 120°, 60° on either side of the vertical, the time for one complete oscillation (2 × 120°) being about 4 s and the test duration being 5 min.		N/A
	The enclosure is then turned through a horizontal angle of 90° and the test is continued for a further 5 min.		N/A
b) spray nozzle	Water flow rate 10 l/min ± 5 %		N/A
	Spray ± 60° from vertical		N/A
	The test duration is 1 min/m ² of the calculated surface area of the enclosure (excluding any mounting surface), with a minimum duration of 5 min.		N/A
14.2.4	Test for second characteristic numeral 4 with oscillating tube or spray nozzle	IPX5	N/A
a) oscillating tube	Water flow rate 0,07 l/min ± 5 % per hole, multiplied by number of holes		N/A

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict
	The oscillating tube has spray holes over the whole 180° of the semicircle.		N/A
	The tube is caused to oscillate through an angle of almost 360°, 180° on either side of the vertical, the time for one complete oscillation (2 × 360°) being about 12 s.		N/A
	The duration of the test is 10 min.		N/A
b) spray nozzle	Water flow rate 10 l/min ± 5 %		N/A
	Spray ± 180° from vertical		N/A
	The test duration is 1 min/m ² of the calculated surface area of the enclosure (excluding any mounting surface), with a minimum duration of 5 min.		N/A
14.2.5	Test for second characteristic numeral 5 with the 6,3 mm nozzle		P
	delivery rate: 12,5 l/min ± 5 %;		P
	core of the substantial stream: circle of approximately 40 mm diameter at 2,5 m distance from nozzle;		P
	test duration per square metre of enclosure surface area likely to be sprayed: 1 min; minimum test duration: 3 min;		P
	distance from nozzle to enclosure surface: between 2,5 m and 3 m.		P
14.2.6	Test for second characteristic numeral 6 with the 12,5 mm nozzle	IPX5	N/A
	delivery rate: 100 l/min ± 5 %;		N/A
	core of the substantial stream: circle of approximately 120 mm diameter at 2,5 m distance from nozzle;		N/A
	test duration per square metre of enclosure surface area likely to be sprayed: 1 min; minimum test duration: 3 min;		N/A
	distance from nozzle to enclosure surface: between 2,5 m and 3 m.		N/A
14.2.7	Test for second characteristic numeral 7: temporary immersion between 0,15 m and 1 m	IPX5	N/A
	the lowest point of enclosures with a height less than 850 mm is located 1 000 mm below the surface of the water		N/A

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict
	the highest point of enclosures with a height equal to or greater than 850 mm is located 150 mm below the surface of the water;		N/A
	the duration of the test is 30 min;		N/A
	the water temperature does not differ from that of the equipment by more than 5 K.		N/A
14.2.8	Test for second characteristic numeral 8: continuous immersion subject to agreement	IPX5	N/A
	the test conditions are subject to agreement between manufacturer and user, but they shall be more severe than those prescribed in 14.2.7		N/A
14.2.9	Test for second characteristic numeral 9 by high pressure and temperature water jetting	IPX5	N/A
	a) For small enclosures (largest dimension less than 250 mm), the enclosure shall be mounted on the test device shown in Figure 12. – turntable speed: 5 r/min ± 1 r/min – spray positions: 0°, 30°, 60°, 90° The test duration is 30 s per position.		N/A
	b) For large enclosures (largest dimension greater than or equal to 250 mm), the enclosure shall be mounted as per intended use. The entire exposed surface area of the enclosure shall be subjected to the spray at some point during the test procedure. – spray positions: the enclosure shall be sprayed from all practical directions covering the entire surface area and the spray shall be, as far as possible, perpendicular to the sprayed surface. – distance between nozzle and sample under test shall be 175 ± 25 mm. The test duration is 1 min/m ² of the calculated surface area of the enclosure (excluding any mounting surface), with a minimum duration of 3 min.		N/A
14.3	Acceptance conditions		P

IEC 60529			
Clause	Requirement + Test	Result - Remark	Verdict
	<p>In general, if any water has entered, it shall not:</p> <ul style="list-style-type: none"> - be sufficient to interfere with the correct operation of the equipment or impair safety; - deposit on insulation parts where it could lead to tracking along the creepage distances; - reach live parts or windings not designed to operate when wet; - accumulate near the cable end or enter the cable if any. 	No water entered	P
	<p>If the enclosure is provided with drain-holes, it should be proved by inspection that any water which enters does not accumulate and that it drains away without doing any harm to the equipment.</p>	No drain-holes	N/A

Appendix 1 Product photos



Photo 1 - Front view



Photo 2 - Rear view

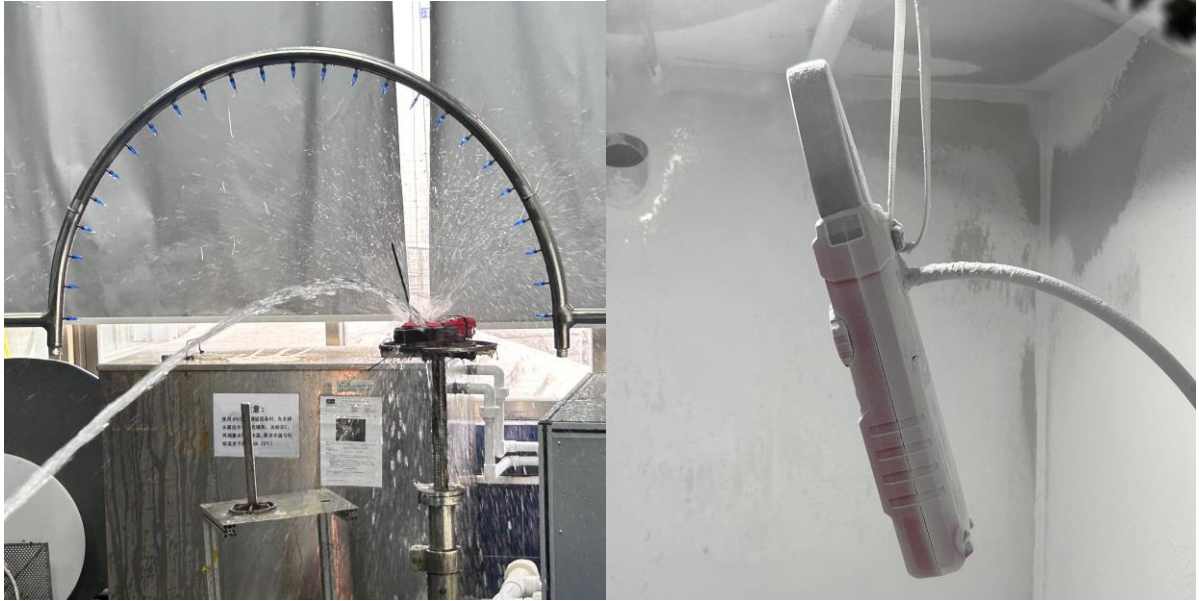


Photo 3 – During testing

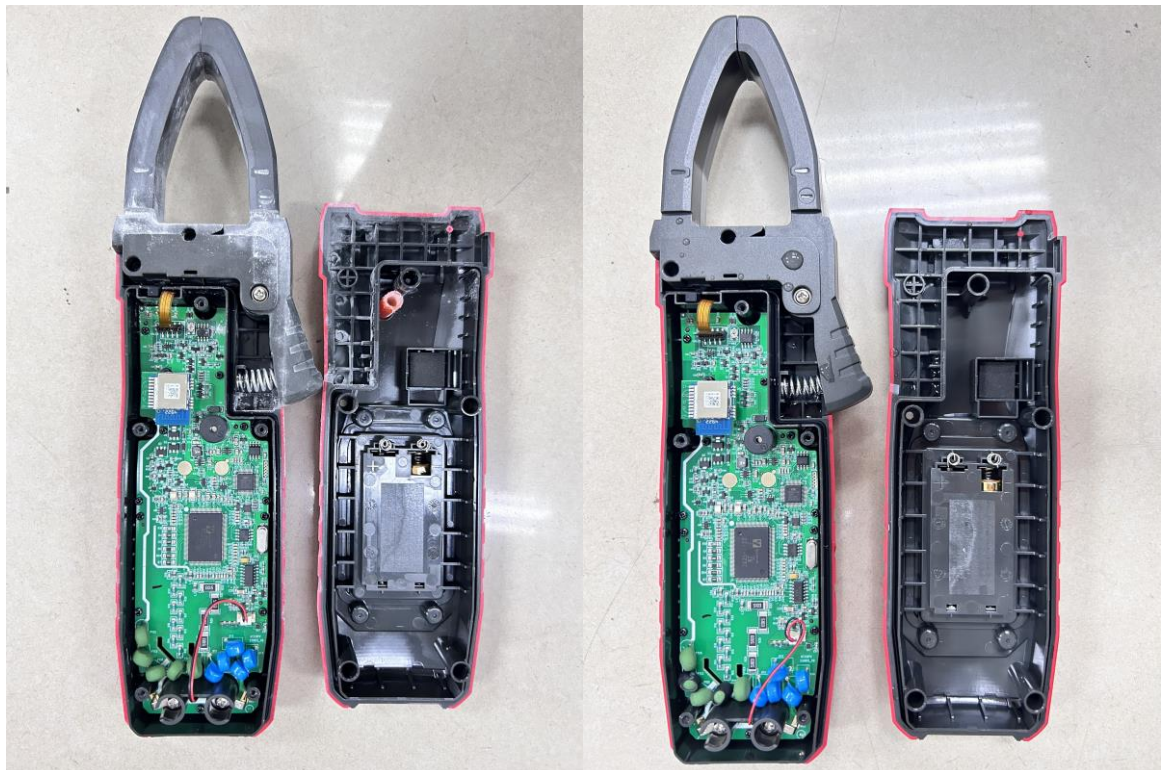


Photo 4 – After test

****END OF REPORT****